#### Components

Standard accessories CoolSpeK main body

A silicon tube ( $\phi 5 \times \phi 9$ , 3m) Temperature controller

Tube sets for gas flow Liquid nitrogen reservoir

(urethane tube, connector of taper pipe threads, flow valve)

User's manual

Outer size of the CoolSpeK main body (without options) 162.5mm (Height) × 90mm (Width) × 111mm (Length)

### Specifications

\*cuvette is not supplied

Liquid nitrogen reservoir : Stainless, 2 Litre

Low-temperature sample chamber : Aluminum, polyurethane foam for thermal insulation

Optical windows : Quartz, Three-way

Suitable cell : Outer dimension of 12.5mm  $\times$  12.5mm

Temperature control : Regulated liq.N2 flow

: (standard) -80°C to room temperature Temperature range

(optional) -80°C to 100°C

Volume of Liq.N2 consumption : 1Litre/hour

Precision of temperature control : ±1°C or ±0.5% of indication value, whichever is greater (error of the sensor not included)

Quantity of dew condensation : Less than 0.10D/hour at -80°C with Unisoku spectrophotometer


: Resistance thermometer sensor (Pt-100 Class B) Temperature sensor **Functions** : There are two built-in heaters in the main body.

One is for prevention of dew condensation on optical windows. Another is for temperature control.


System electronics : AC100V 1A (Transformer will be provided accordance with the voltage of destination country.)


Cryogen used

## Application Examples



Spectral changes for the reaction of  $O_2$ and a Cu(I) complex at -80 °C Formation of a m-peroxo dinuclear copper(II) complex can be easily monitored by the time-dependent UV-vis spectrum at low temperature (Courtesy of Prof. Shinobu Itoh of

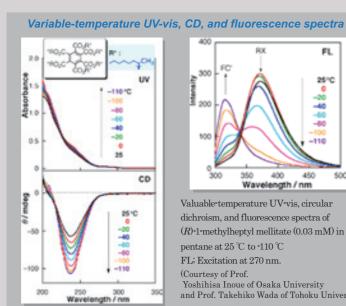



# UNISOKU Scientific Instruments **UnispeKs**

Osaka University)


## Unisoku Co.,Ltd.

2-4-3, Kasugano, Hirakata, Osaka 573-0131, Japan TEL:+81-72-858-6456 FAX:+81-72-859-5655 e-mail:info@unisoku.co.jp URL:http://www.unisoku.co.jp URL:http://www.unisoku.com

Acknowledgement: These instrument components are subject to change without prior notice for improvement in performance.





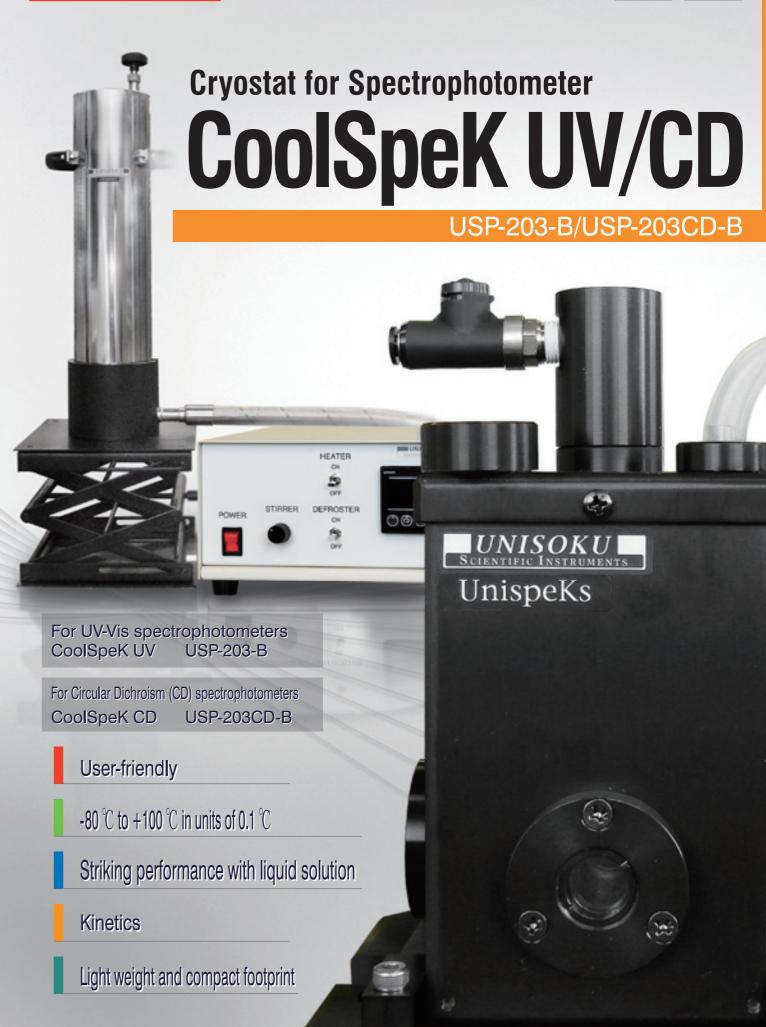



Agilent 8453-Series Diode Array Spectrophotometer Beckman DU-7400 Spectrophotometer Edinburgh Instruments Fluorescence Spectrometer JASCO Spectrophotometer V-550/560/570 V-650/660/670 JASCO Fluorescence Spectrophotometer FP-6500 JASCO Circular Dichroism Dispersion Measurement System J-720/820 Hewlett-Packard HP8453-Series Diode Array Spectrophotometer Hitachi Spectrophotometer U-3500

Shimadzu Spectrophotometer UV-2400/2450/2550 Shimadzu Fluorescence Spectrophotometer RF-5300\*(1) Varian Spectrophotometer Cary50

\* In some spectrophotometers, room light may get into detectors when the cryostat is attached. \*Please contact us if your spectrophotometer is not listed above.

\*(1)Magnetic stirrer(No.CS-ST) can not be installed for RF-5300.

(light path length: 10mm)



# Magnetic stirring bar (No.CS-SB)

This is used in the Standard Cuvette (No.CS-CL-U1). Specified Tolerance of Teflon® Walls High Strength Magnetization



Suitable dimension: q10mm or 10mmx10mm, Thickness: 0.5-1.5mm Please contact us if your sample dimension is different from above.

## Solid sample holder (for fluorescence) (No.CS-KF-H5-27)

Suitable sample: solid sheet or powder

Suitable dimension: \phi13mmx13mm, Thickness: 0.5-2.5mm Please contact us if your sample dimension is different from above.

